


Tue Feb 24 08:44:19 2004


TIDE Mass_0

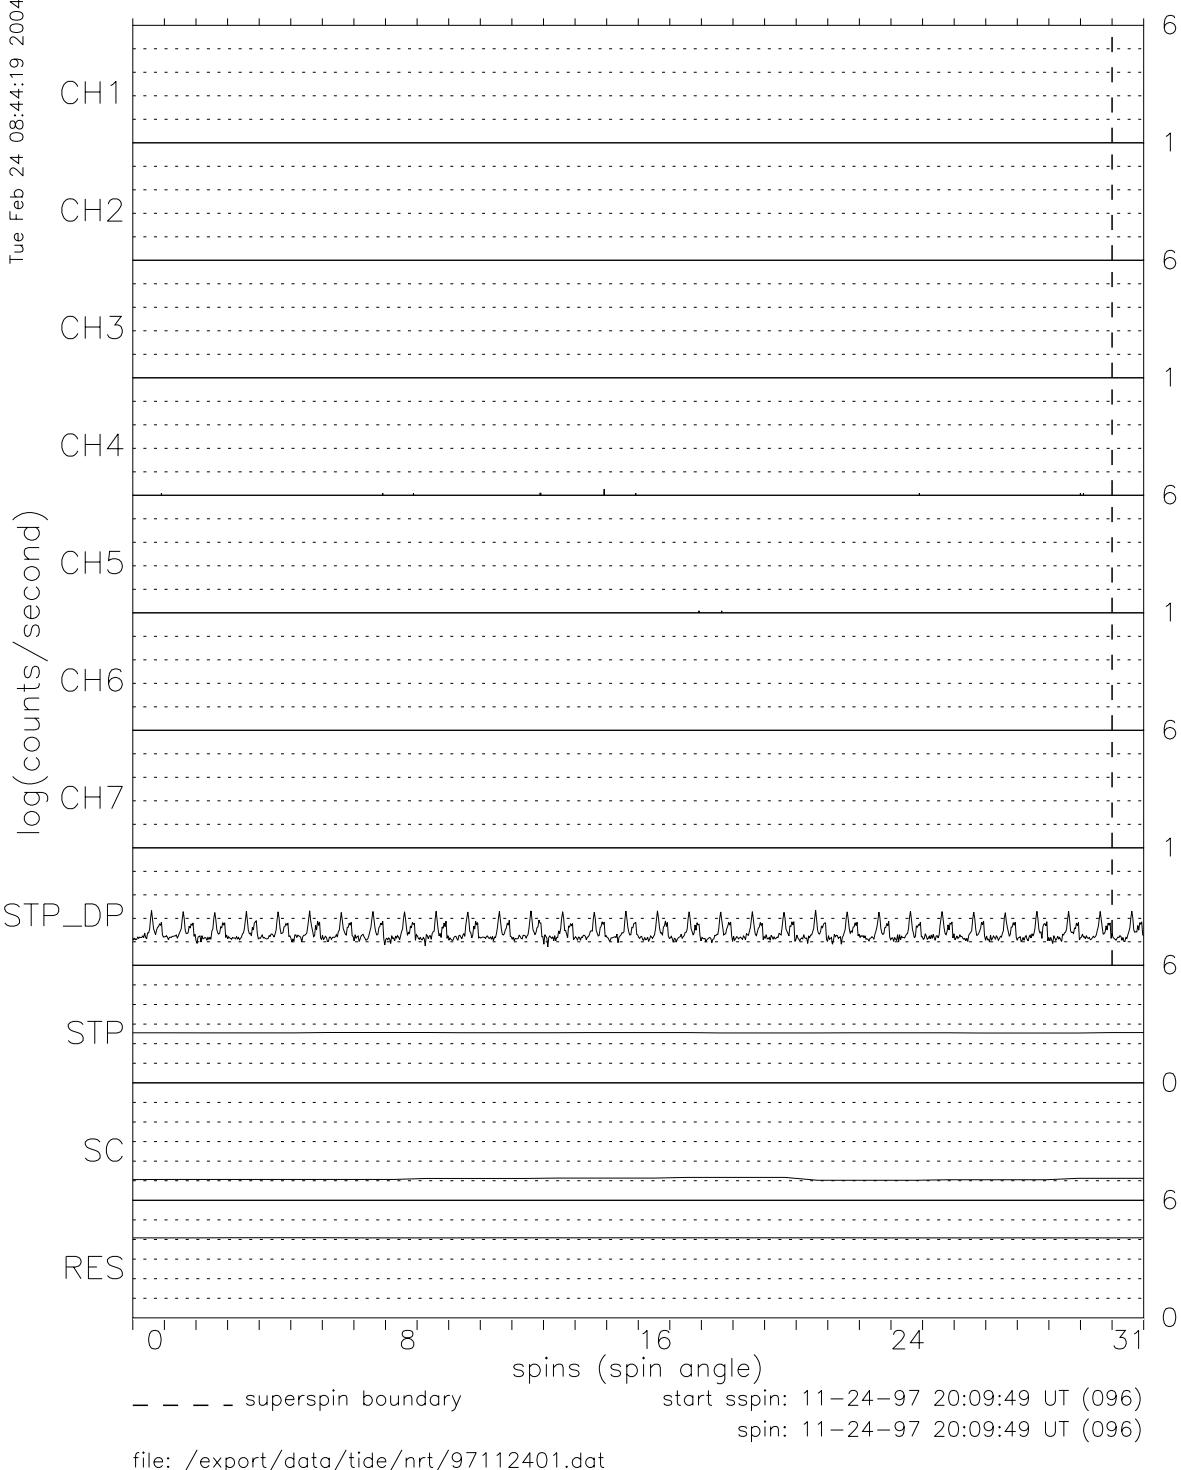

-15kV TOF: -9116 v
-3.6kV MCP: -2593 v
-2.4kV MCP: -1579 v
Input Cur: 294 ma
RPA max: 237 v
Mirror max: 238 v

Tue Feb 24 08:44:19 2004

TIDE Direct Events

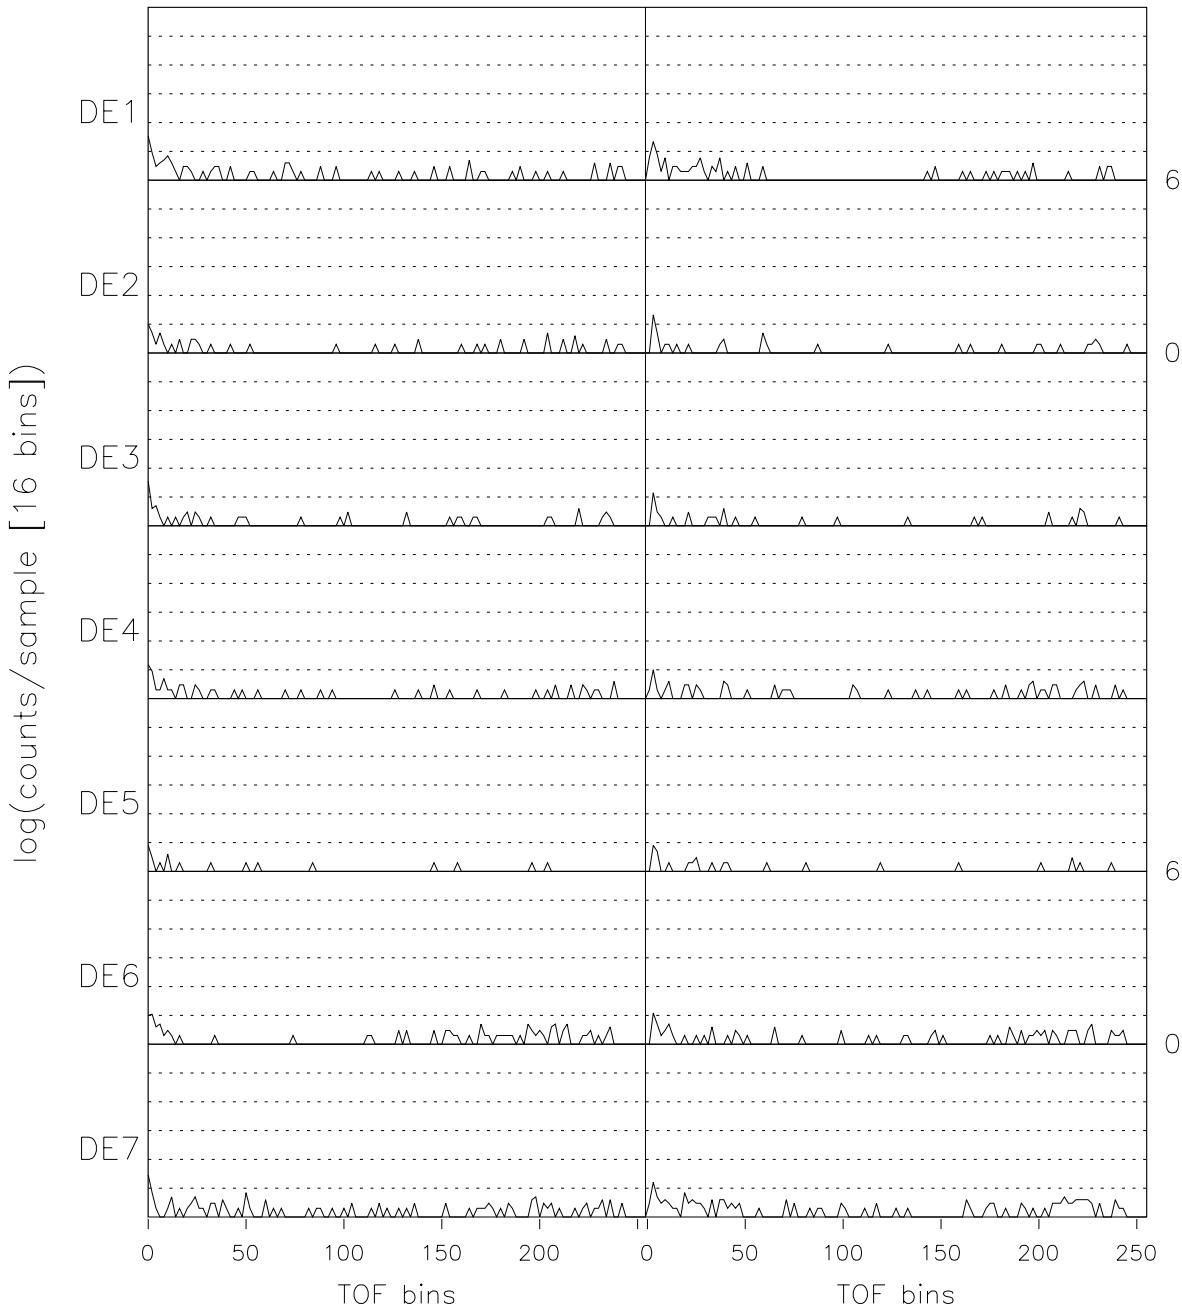

reported: 11-24-97 20:03:19 UT

reported: 11-24-97 20:06:31 UT

file: /export/data/tide/nrt/97112401.dat

-15kV TOF: -9181 v

-3.6kV MCP: -2578 v

-2.4kV MCP: -1579 v

Input Cur: 302 ma

RPA max: 237 v

Mirror max: 238 v